Instruction Guide | **Accessory Mounting Rail f/Accutron™ RFS™**

U.S. & Canada (888) 520-4998 | International (801) 875-4998 | www.**MTI**.net

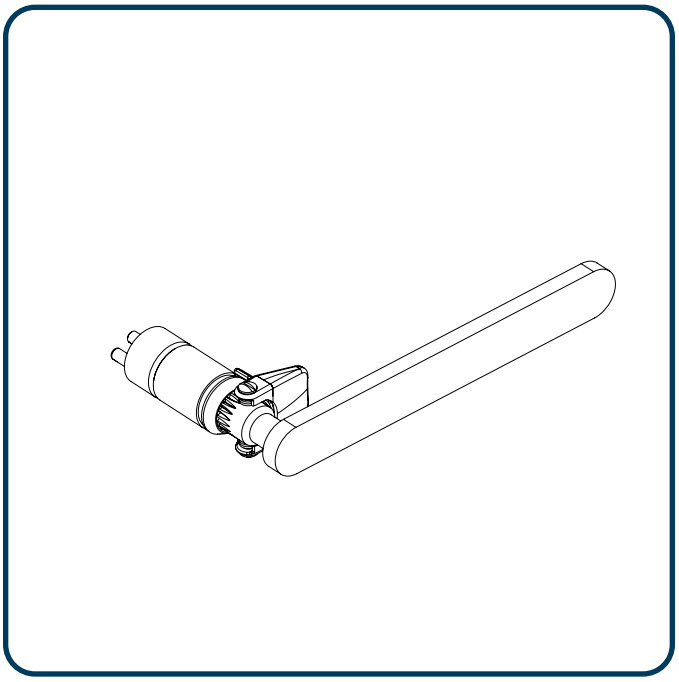

Required Tools

	3/16" Allen® Wrench

⚠ *WARNING/AVERTISSEMENT*

Read this manual before installation and use.

Lisez ce manuel avant l'installation et l'utilisation.

⚠ *WARNING/AVERTISSEMENT*

No modification of this equipment is allowed.

Aucune modification de cet équipement est autorisé.

⚠ *WARNING/AVERTISSEMENT*

This mounting rail has been tested to fit the Accutron™ RFS™ Remoote Flow System. Do not attach any other devices to this mounting rail. The warnings and instructions contained in this guide pertain solely to the Accessory Mounting Rail Assembly. Users must also comply with all instructions and warnings provided with the Accutron RFS system to ensure safe and proper operation.

Ce rail de montage a été testé pour s'adapter au système Accutron™ RFS™. Ne fixez aucun autre dispositif sur ce rail de montage. Les avertissements et instructions contenus dans ce guide concernent uniquement l'ensemble du rail de montage pour accessoires. Les utilisateurs doivent également se conformer à toutes les instructions et à tous les avertissements fournis avec le système Accutron RFS afin d'en garantir un fonctionnement sûr et correct.

⚠ *WARNING/AVERTISSEMENT*

Ensure equipment, patient, and other objects are in safe condition before operating the equipment.

Assurer l'appareil, patient, et d'autre objets sont dans un état sûr avant d'utiliser l'appareil.

⚠ *WARNING/AVERTISSEMENT*

This product can expose you to chemicals including nickel, which is known to the State of California to cause cancer. For more information go to www.P65Warnings.ca.gov and see www.mti.net/faqs for details on California Proposition 65.

Ce produit peut vous exposer à des agents chimiques, y compris le nickel, identifiés par l'État de Californie comme pouvant causer le cancer. Pour de plus d'informations, prière de consulter www.P65Warnings.ca.gov et voir www.mti.net/faqs pour les détails sur le Proposition de Californie 65.

This manual is for the following product numbers:

PRODUCT NUMBER	DESCRIPTION
130-4491	Accessory Mtg Rail Assy, Base Mtd G2

REVISION HISTORY TABLE

DATE	REVISION	CO#/ECO#	DETAILS
8/18/2026	A	CO-0669/EC-0833	Initial release

⚠ *WARNING/AVERTISSEMENT*

This accessory is only for use on the following MTI standard base chair models: 722-001-80, 729-001-80, 829-001-80, 830-001-80.

Cet accessoire ne doit être utilisé qu'avec les modèles de fauteuils MTI à base standard suivants : 722-001-80, 729-001-80, 829-001-80, 830-001-80.

⚠ *WARNING/AVERTISSEMENT*

Only attach an Accutron™ RFS™ Remote Flow System to this rail accessory.

Ne fixez le système Accutron™ RFS™ qu'à cet accessoire de montage sur rail.

INSTALLATION

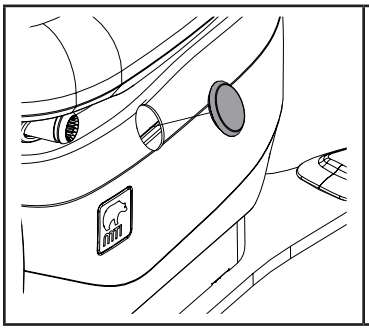

1. To prepare the chair for the accessory:

Remove the oval hole plug in the base cover from the side where the accessory will be attached.

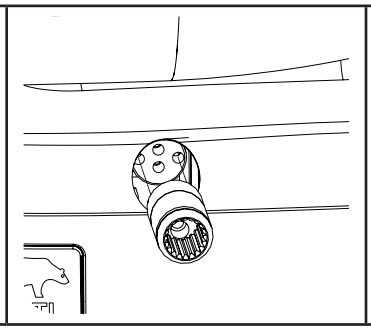

2. To attach the spline assembly:

Orient the pins of the spline assembly horizontally.

Insert the spline assembly through the opening in the cover and insert the pins into the holes in the mount inside the base cover.

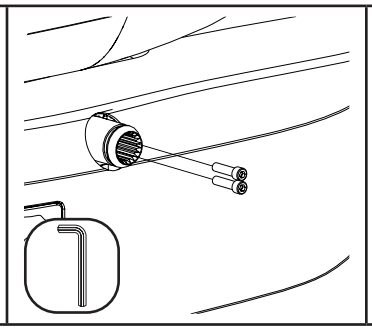

3. Secure the spline assembly with the (2) 1/4-20 x 1" cap screws using a 3/16" Allen® wrench.

The preferred tool is a T-handle Allen® wrench for better leverage.

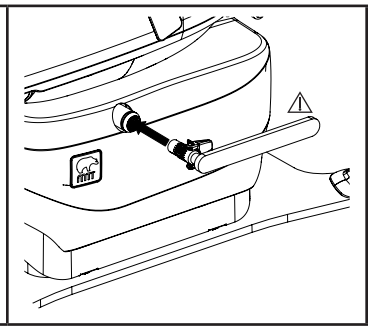

4. To attach the rail to the spline assembly:

Insert the mail spline of the rail into the female spline socket. The rail must be oriented parallel to the floor facing the rear of the chair as shown.

NOTE: Follow the Accutron™ RFS™ Chair Mount Installation Instructions for proper installation of the Accutron™ RFS™ to the accessory mounting rail.

⚠ *WARNING/AVERTISSEMENT*

Only insert the rail in the spline so it is parallel to the floor and oriented towards ther rear of the chair. Failure to orient the rail properly will cause damage to the chair or Accutron™ RFS™ Remote Flow System.

Insérez le rail dans la rainure de manière à ce qu'il soit parallèle au sol et orienté vers l'arrière du fauteuil. Une mauvaise orientation du rail endommagera le fauteuil ou le système Accutron™ RFS™.

EXPLODED VIEWS

130-4491 ACCESSORY MTG RAIL ASSY, BASE MTD G2

PART NUMBER	QTY	DESCRIPTION
130-0322	1	FEMALE SPLINE WLD, A SIZE
130-1715	1	TRIGGER LATCH, SPLINE MTD
130-1290	1	TORSION SPRING, TRIGGER LATCH
130-2010	1	BINDING SCREW SET, 1/4 X 1-1/2, 10-24 X 11/16, BLACK PLASTIC
130-4605	1	ACCESSORY MTG RAIL WLD, 829 SEAT & 830 BACK/SEAT G2
029587	2	SHC SCREW, 1/4-20 x 1, BLACK

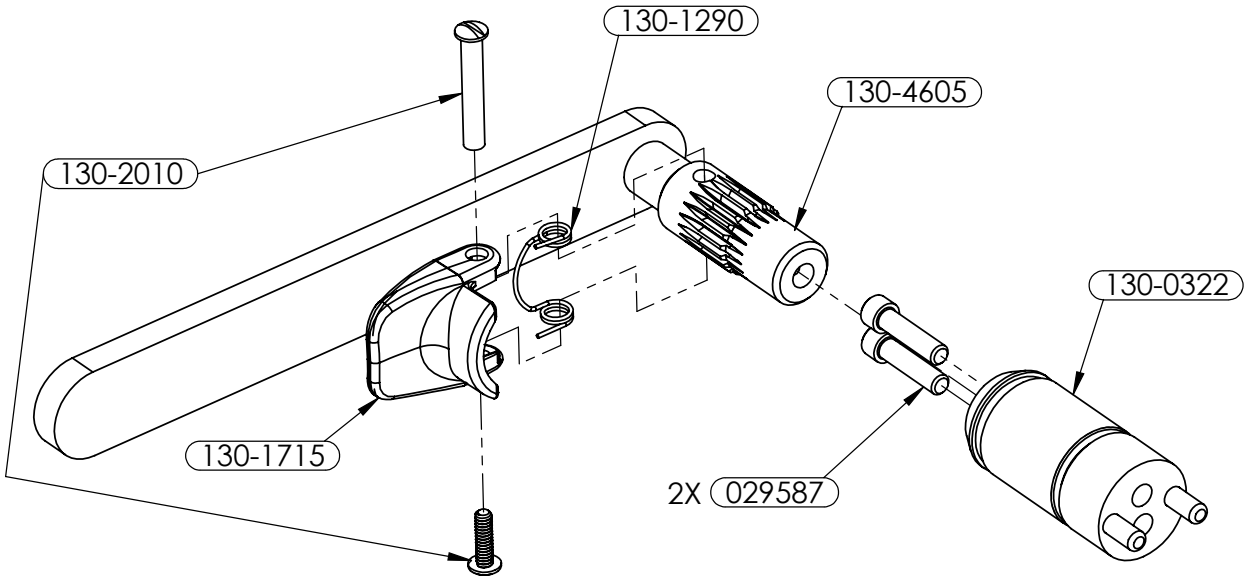

Instruction Guide | **Accessory Mounting Rail f/Accutron™ RFS™**

U.S. & Canada (888) 520-4998 | International (801) 875-4998 | www.**MTI**.net

DISINFECTION

Follow the current CDC Guideline for Disinfection & Sterilization in Healthcare Facilities or other local guidelines.

MTI understands that many customers prefer to use a pre-mixed disinfecting solution in a spray or wipe. It is MTI's recommendation not to use sprays because over time the overspray will cause damage to the surfaces if not immediately wiped up. See "MTI Suggested Disinfectants Policy" for more details on disinfecting solutions which have been tested on MTI's products. It is available for download at www.mti.net/disinfectantspolicy. In the U.S. & Canada, call (888) 520-4998, or International call (801) 875-4998, or email customer.service@mti.net to request a copy.

CLEANING

These instructions apply only to the Base Mtd Accessory Mtg Rail. Surfaces should be wiped down with a quality grade cleaner and a soft cloth or a damp cloth with mild soap.

Calls for Service

(877) 875-4990 | International (801) 875-4990
technical.support@mti.net | www.mti.net

LIMITED WARRANTY

Medical Technology Industries, Inc. (hereinafter referred to as MTI), shall repair or replace products of its manufacture, which prove to be defective in material and/or workmanship for a period of twelve (12) months from the date of shipment to the customer (the "Warranty Period"). MTI will, at its option, provide parts to the customer or repair the defective part at MTI's factory or authorized repair facility. Except as it may otherwise specifically agree in writing, MTI shall not be liable for transportation or labor charges for repairs or adjustments or other work done on any of its products by MTI's authorized dealers or service organizations.

Customer shall notify MTI of any alleged claim or defect within fourteen (14) days from the date customer discovers, or upon reasonable inspection should have discovered, such alleged claim or defect (but in any event before the expiration of the Warranty Period). All repair parts are warranted for Ninety (90) calendar days from the date of shipment to the customer. Warranty is non-cumulative.

This warranty does not apply to any part or product which upon examination by MTI or its authorized agents indicates the product has been repaired or altered in any way by persons other than MTI or its authorized agents, has been misused, abused or used in a manner contrary to any instructions issued by MTI. Any parts or products claimed under this warranty must be properly packaged by customer and returned to MTI's factory with no liability to MTI for the parts, products or transportation charges thereon.

In no event, shall MTI have any liability for consequential, indirect, incidental, special, exemplary, punitive or enhanced damages, lost profits or diminution in value arising out of or relating to a product defect or the repair or replacement of any products manufactured or sold by it.

THE FOREGOING LIMITED WARRANTY IS MADE IN LIEU OF ALL WARRANTIES EXPRESSED OR IMPLIED, AND MTI MAKES NO OTHER WARRANTY WHATSOEVER WITH RESPECT TO THE PRODUCTS INCLUDING BUT NOT LIMITED TO, ANY IMPLIED WARRANTY OR MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.

MTI, Inc.
3655 W Ninigret Drive
Salt Lake City, Utah, 84104-6572
800-924-4655 • 801-875-4999 • Fax 801-952-0548
www.mti.net

© MTI, Inc. All rights reserved. MTI reserves the right to make any product changes without notice. The MTI brand and Bear logo design are registered trademarks of MTI, Inc. in the United States.

130-4553 Rev A

Specialized Equipment for Specialty Healthcare